


IMPELLA® IS THE MOST BLOOD COMPATIBLE HEART PUMP

Ratio of Device Plasma Free Hemoglobin to Static Blood
(standard FDA bench test measured at 6 hrs)

RBC
Damage

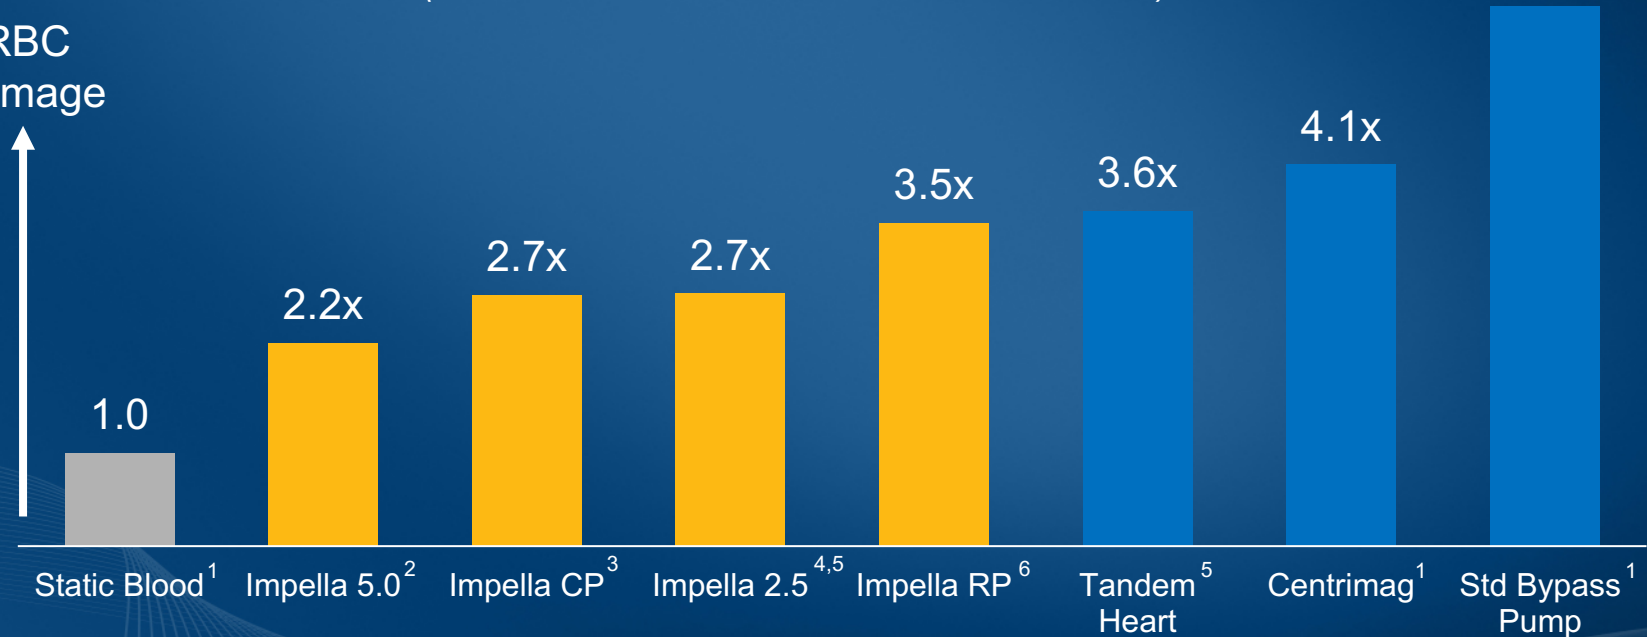

1. CentriMag/Industry standard data – Levitronix Website

2. FDA Bench Test Data for Impella 5.0®/Impella LD® PMA P140003

3. FDA Bench Test Data for Impella CP® PMA Supplement P140003/S004

4. FDA Bench Test Data for Impella 2.5® PMA P140003

5. FDA Bench Test Data for Impella 2.5 510(k) Clearance K063723

6. FDA Bench Test Data for Impella RP® PMA P170011

IMPELLA® DEVICE INDICATION & SAFETY INFO.

INDICATIONS FOR USE

High-Risk PCI

The Impella 2.5®, Impella CP® and Impella CP® with SmartAssist® Systems are temporary (≤ 6 hours) ventricular support devices indicated for use during high-risk percutaneous coronary interventions (PCI) performed in elective or urgent, hemodynamically stable patients with severe coronary artery disease, when a heart team, including a cardiac surgeon, has determined high-risk PCI is the appropriate therapeutic option. Use of the Impella 2.5, Impella CP, and Impella CP with SmartAssist Systems in these patients may prevent hemodynamic instability, which can result from repeat episodes of reversible myocardial ischemia that occur during planned temporary coronary occlusions and may reduce peri- and post-procedural adverse events.

Cardiogenic Shock

The Impella 2.5®, Impella CP®, Impella CP® with SmartAssist®, Impella 5.0® and Impella LD® Catheters, in conjunction with the Automated Impella® Controller (collectively, "Impella® System Therapy"), are temporary ventricular support devices intended for short term use (≤ 4 days for the Impella 2.5, Impella CP, and the Impella CP with SmartAssist, and ≤ 14 days for the Impella 5.0, and Impella LD) and indicated for the treatment of ongoing cardiogenic shock that occurs immediately (< 48 hours) following acute myocardial infarction or open heart surgery or in the setting of cardiomyopathy, including peripartum cardiomyopathy, or myocarditis as a result of isolated left ventricular failure that is not responsive to optimal medical management and conventional treatment measures (including volume loading and use of pressors and inotropes, with or without IABP). The intent of Impella System Therapy is to reduce ventricular work and to provide the circulatory support necessary to allow heart recovery and early assessment of residual myocardial function.

Important Risk Information for Impella devices

CONTRAINDICATIONS

The Impella 2.5, Impella CP, Impella CP with SmartAssist, Impella 5.0 and Impella LD are contraindicated for use with patients experiencing any of the following conditions: Mural thrombus in the left ventricle; Presence of a mechanical aortic valve or heart constrictive device; Aortic valve stenosis/calcification (equivalent to an orifice area of 0.6 cm² or less); Moderate to severe aortic insufficiency (echocardiographic assessment graded as $\geq +2$); Severe peripheral arterial disease precluding placement of the Impella System; Significant right heart failure*; Combined cardiorespiratory failure*; Presence of an Atrial or Ventricular Septal Defect (including post-infarct VSD)*; Left ventricular rupture*; Cardiac tamponade*

** This condition is a contraindication for the cardiogenic shock indication only.*

POTENTIAL ADVERSE EVENTS

Acute renal dysfunction, Aortic valve injury, Bleeding, Cardiogenic shock, Cerebral vascular accident/Stroke, Death, Hemolysis, Limb ischemia, Myocardial infarction, Renal failure, Thrombocytopenia and Vascular injury

In addition to the risks above, there are other **WARNINGS** and **PRECAUTIONS** associated with Impella devices. Visit <http://www.abiomed.com/important-safety-information> to learn more.

RIGHT-SIDE SUPPORT – INDICATION & SAFETY INFO.

INDICATIONS FOR USE

The Impella RP® System is indicated for providing temporary right ventricular support for up to 14 days in patients with a body surface area $\geq 1.5 \text{ m}^2$, who develop acute right heart failure or decompensation following left ventricular assist device implantation, myocardial infarction, heart transplant, or open-heart surgery.

Important Risk Information for Impella RP System

CONTRAINDICATIONS

The Impella RP System is contraindicated for patients with the following conditions: Disorders of the pulmonary artery wall that would preclude placement or correct positioning of the Impella RP device. Mechanical valves, severe valvular stenosis or valvular regurgitation of the tricuspid or pulmonary valve. Mural thrombus of the right atrium or vena cava. Anatomic conditions precluding insertion of the pump. Presence of a vena cava filter or caval interruption device, unless there is clear access from the femoral vein to the right atrium that is large enough to accommodate a 22 Fr catheter.

POTENTIAL ADVERSE EVENTS

The potential adverse effects (eg, complications) associated with the use of the Impella RP System: Arrhythmia, Atrial fibrillation, Bleeding, Cardiac tamponade, Cardiogenic shock, Death, Device malfunction, Hemolysis, Hepatic failure, Insertion site infection, Perforation, Phlegmasia cerulea dolens (a severe form of deep venous thrombosis), Pulmonary valve insufficiency, Respiratory dysfunction, Sepsis, Thrombocytopenia, Thrombotic vascular (non-central nervous system) complication, Tricuspid valve injury, Vascular injury, Venous thrombosis, Ventricular fibrillation and/or tachycardia.

In addition to the risks above, there are other **WARNINGS** and **PRECAUTIONS** associated with Impella RP.

Visit www.abiomed.com/important-safety-information to learn more.